

June 2024

VOLUNTARY MEDICAL DEVICE SAFETY ALERT**SPECTRA OPTIA™ APHERESIS SYSTEM
Reminder to Prime Blood Warmers**

Dear Valued Customer:

The purpose of this letter is to remind Spectra Optia system users of a potential safety hazard when using a blood warmer attached to a Spectra Optia tubing set and to reinforce the actions required to mitigate this risk. If the blood warmer is not primed before use, air could be delivered to a patient.

Many Spectra Optia procedures include the option to use a blood warmer. The Spectra Optia operator's manual instructs operators how to connect and prime a blood warmer when one is used. The operator's manual also includes warnings about the risk of delivering air to a patient if a blood warmer is not primed. These warnings appear throughout the manual: in the "General procedural warnings" section in the Preface of the operator's manual and in the instructions for priming the lines before connecting the patient for each procedure for which a blood warmer is an option.

If an operator did not observe this warning and/or did not follow the instructions in the operator's manual, this safety hazard could occur.

REASON FOR THE SAFETY ALERT

Terumo Blood and Cell Technologies has received complaints where air was returned to a patient due to an unprimed blood warmer. A blood warmer that is not primed and is connected to the Spectra Optia tubing set return line could cause a risk.

A blood warmer can be attached to the tubing set either at the beginning of a procedure or during a procedure.

Terumo BCT, Inc.

10811 West Collins Ave.
Lakewood, Colorado 80215-4440
USA
USA Phone: 1.877.339.4228
Phone: +1.303.231.4357
Fax: +1.303.542.5215

Terumo BCT Europe N.V.

Europe, Middle East and Africa
Ikaroslaan 41
1930 Zaventem
Belgium
Phone: +32.2.715.0590
Fax: +32.2.721.0770

Terumo BCT Asia Pte. Ltd.

89 Science Park Drive
#04-25 (Lobby B)
The Rutherford
Singapore 118261
Phone: +65.6715.3778
Fax: +65.6774.1419

Terumo BCT Latin America S.A.

La Pampa 1517-12th Floor
C1428DZE
Buenos Aires
Argentina
Phone: +54.11.5530.5200
Fax: +54.11.5530.5201

Terumo BCT Japan, Inc.

Tokyo Opera City Tower 49F,
3-20-2, Nishi-Shinjuku,
Shinjuku-ku, Tokyo 163-1450,
Japan
Phone: +81.3.6743.7890
Fax: +81.3.6743.9800

PROCEDURAL CONSIDERATIONS

- **Scenario 1: The operator attaches a blood warmer to the return line at the beginning of the procedure. In this scenario, the operator sees the screen shown in Figure 1.** The text and graphics instruct the operator to connect the blood warmer. The text that instructs the operator to prime the blood warmer is circled for illustration purposes in Figure 1.

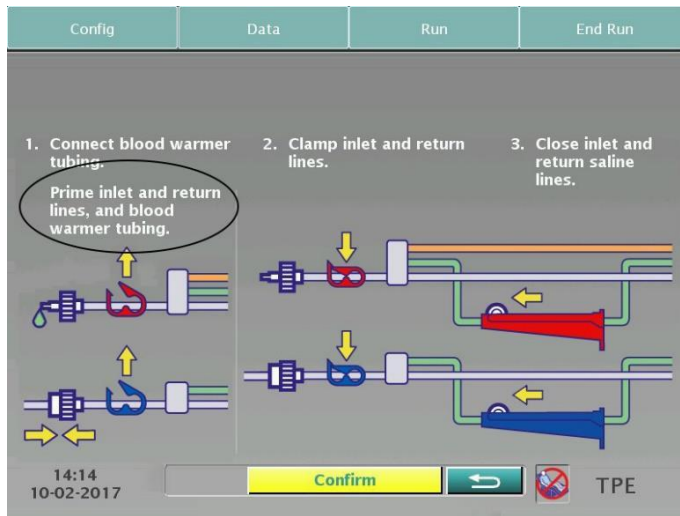


Figure 1. Screen instructs the operator to prime the blood warmer tubing

- **Scenario 2: The operator connects a blood warmer to the return line in the latter stages of system prime but before the patient is connected OR the operator connects a blood warmer to the return line mid-procedure.** In this scenario, the text that instructs the operator to connect the blood warmer and to prime the blood warmer tubing does not appear, as shown in Figure 2.

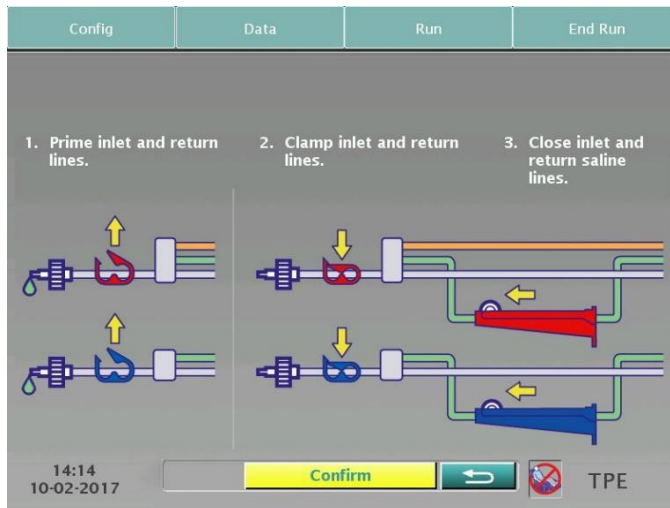


Figure 2. Screen does not instruct the operator to prime the blood warmer tubing. If an operator connects a blood warmer mid-run but fails to prime the blood warmer tubing set and continues to connect the patient and resumes the procedure, any air in the blood warmer tubing set will be returned to the patient.

RISK TO THE PATIENT

The population at most risk are patients ≤ 20 kg and those with underlying cardiopulmonary issues. Unprimed blood warmer tubing could result in air being returned to the patient when the procedure is started or resumed, resulting in a venous air embolism.

A venous air embolism is the collection of air within the systemic venous circulation, which can affect blood flow. To produce symptoms, it is estimated that more than 5 mL/kg of air must be introduced into the venous system; however, complications can occur with 20 mL of air. Therefore, any person receiving the volume of air of the blood warmer tubing could experience the full range of effects, up to and including death.

ACTIONS BEING TAKEN BY TERUMO BLOOD AND CELL TECHNOLOGIES

Terumo Blood and Cell Technologies is notifying you that a system reminder to prime the blood warmer may not always be provided in screen instructions.

Please follow the Operator's Manual.

ACTIONS REQUIRED BY HEALTHCARE PROVIDERS AND DISTRIBUTORS

1. Distribute this notification to all Spectra Optia system users within your organization.
2. Continue to use your Spectra Optia system(s) in accordance with the operator's manual and the operator training materials.
3. When you configure the use of a blood warmer for the tubing set return line, the instructions to connect the blood warmer are displayed on the screen before you connect the patient. You must prime the blood warmer tubing set before you connect the patient. Please refer to Spectra Optia system operator's manual, "Configuring the Use of a Blood Warmer."
4. In the "Selecting Procedure Options" section of the operator's manual, follow the updated instructions to indicate the use of a blood warmer during the procedure. You must prime the blood warmer tubing set before you connect the patient.
5. **IMPORTANT:** Complete the attached acknowledgement and fax or email the acknowledgement to Terumo Blood and Cell Technologies by **August 31, 2024**. Your return of the acknowledgement is critical so that we can confirm that you have received the Safety Alert.

CONTACT INFORMATION

Terumo Blood and Cell Technologies is dedicated to providing you with the highest quality support and communicating information regarding our products. If you have any questions, please contact your Terumo Blood and Cell Technologies representative or your regional Customer Support Center.

Sincerely,

Scot Hilden
Quality Manager

Terumo Blood and Cell Technologies
Unlocking Potential