

Recommendations for treatment with

 **EYLEA® 40 mg/mL**
solution for injection
aflibercept

 **EYLEA® 114.3 mg/ml**
solution for injection
aflibercept

Prescriber Guide

This Guide provides important information on EYLEA® 40mg/ml solution for injection (2 mg aflibercept dose) and EYLEA® 114.3 mg/ml solution for injection (8 mg aflibercept dose), the medication itself, and how to correctly administer it to your patients.

Please provide the adult patient or the parent/caregiver with the EYLEA® Patient Information Leaflet. In addition, please also provide the adult patient with the EYLEA® patient guide, including its audio version (read out of the patient guide). The above information is available on <https://www.edumaterial.bayer.com.mt> including its audio version.

In this document, for the Retinopathy of Prematurity (ROP) indication, patient = preterm infant = premature baby.

For further information and additional details on EYLEA®, please see the Summary of Product Characteristics (SmPC), https://www.ema.europa.eu/en/documents/product-information/eylea-epar-product-information_en.pdf.

Prescriber guide approved by Malta Medicines Authority in April 2026

INTRAVITREAL INJECTION PROCEDURE VIDEO

**EYLEA 40 MG/ML SOLUTION FOR INJECTION (2 MG DOSE)
(PRE-FILLED SYRINGE)**

AND

**EYLEA 114.3 MG/ML SOLUTION FOR INJECTION (8 MG DOSE)
(VIAL)**

**EYLEA 114.3 MG/ML SOLUTION FOR INJECTION (8 MG DOSE)
(PRE-FILLED SYRINGE)**

PLEASE SCAN:



OR VISIT:





<https://www.edumaterial.bayer.com.mt/mt-eylea-pg>

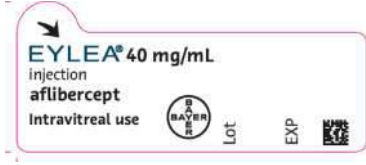
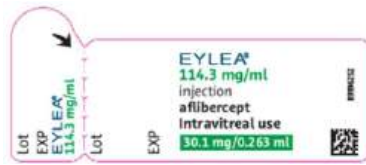




Contents

KEY SUMMARY FOR EYLEA USE IN ADULTS	4
<i>Contraindications.....</i>	<i>5</i>
<i>Key instructions for use in adults.....</i>	<i>5</i>
<i>Selected instructions for storage and handling of EYLEA</i>	<i>6</i>
GENERAL INFORMATION FOR ADULT PATIENTS	6
KEY SUMMARY FOR EYLEA USE IN RETINOPATHY OF PREMATUREITY.....	7
<i>Indication in preterm infants.....</i>	<i>7</i>
<i>Contraindications.....</i>	<i>7</i>
<i>Key instructions for use in ROP.....</i>	<i>7</i>
<i>Selected instructions for storage and handling of EYLEA</i>	<i>8</i>
<i>Dosing recommendations for retinopathy of prematurity:.....</i>	<i>8</i>
GENERAL INFORMATION FOR PARENT/CAREGIVER.....	8
IMPORTANT SAFETY INFORMATION ABOUT EYLEA	8
<i>Special warnings and precautions for use</i>	<i>8</i>
<i>Post-Injection care in Adults.....</i>	<i>12</i>
<i>Post-Injection care in ROP</i>	<i>12</i>
STORAGE AND HANDLING OF EYLEA.....	14
<i>Special precautions for storage of the EYLEA vial and pre-filled syringe.....</i>	<i>16</i>
<i>Storage and handling instructions for the PICLEO paediatric dosing device.....</i>	<i>16</i>
INSTRUCTIONS FOR USE OF EYLEA IN ADULTS.....	17
<i>General preparation for injection.....</i>	<i>17</i>
<i>Pre-filled syringe 40 mg/ml (2 mg dose), solution for injection (for use in adults)</i>	<i>17</i>
<i>Pre-filled syringe 114.3 mg/ml (8 mg dose), solution for injection (for use in adults)</i>	<i>20</i>
<i>Vial 40 mg/ml (2 mg dose) and 114.3 mg/ml (8 mg dose) solution for injection (for use in adults).....</i>	<i>22</i>
<i>Injection Procedure for Adults.....</i>	<i>24</i>
INSTRUCTIONS FOR USE OF EYLEA IN ROP	26
<i>General preparation for injection.....</i>	<i>26</i>
<i>Important information about the PICLEO paediatric dosing device.....</i>	<i>26</i>
<i>Pre-filled syringe (for use in ROP).....</i>	<i>27</i>
<i>Injection Procedure for ROP.....</i>	<i>31</i>

KEY SUMMARY FOR EYLEA USE IN ADULTS

Differences between EYLEA 40 mg/ml solution for injection (2 mg dose) and EYLEA 114.3 mg/ml solution for injection (8 mg dose)

	EYLEA 40 mg/ml	EYLEA 114.3 mg/ml
Presentation	Pre-filled syringe Vial	Pre-filled syringe with OcuClick dosing system Vial
Approved Indications in Adult (18 years and older) patients		
Neovascular wet age-related macular degeneration (AMD)	Yes	Yes
Visual impairment due to diabetic macular oedema (DME)	Yes	Yes
Visual impairment due to macular oedema secondary to retinal vein occlusion (RVO) including branch (BRVO) or central (CRVO)	Yes	Yes*
Visual impairment due to myopic choroidal neovascularisation (mCNV)	Yes	No
Dose per injection	2 mg	8 mg
Injection volume	0.05 ml (50 microlitres)	0.07 ml (70 microlitres)
Packaging		
Vial		

	EYLEA 40 mg/ml	EYLEA 114.3 mg/ml
Label on Vial		
Pre-filled syringe		
Label on pre-filled syringe		
Posology for approved indications	The posology recommendations differ between EYLEA 40 mg/ml and for EYLEA 114.3 mg/ml and between indication. Refer to the SmPC (Section 4.2) for complete information on posology and dosing for EYLEA 40 mg/ml and for EYLEA 114.3 mg/ml	

* Including HRVO: Hemiretinal vein occlusion – Only applicable to **EYLEA 114.3 mg/ml**.
The packaging and labels may vary to a small degree to what is available in Ireland.

Contraindications


- Hypersensitivity to aflibercept or to any of the excipients listed in section 6.1 of the Summary of Product Characteristics (SmPC)
- Active or suspected ocular or periocular infection
- Active severe intraocular inflammation

Key instructions for use in adults

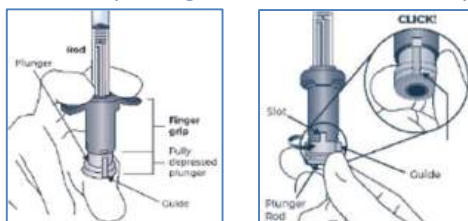
- Each vial/pre-filled syringe is for single use only.
- The vials and the pre-filled syringes come with excess volume. Before injecting, syringes with solution withdrawn from the vial and the pre-filled syringes must be primed to the correct volume for injection according to the steps in the instructions for use.
- The EYLEA 114.3 mg/ml pre-filled syringe (8 mg dose) does not have a dose line because it is designed to set the dose mechanically as shown in the key steps briefly summarised below and provided in detail in the instructions for use section of this guide. Priming and setting the dose must be done using the steps described below and in the instructions for use section.
- Ensure proper aseptic technique including the use of broad-spectrum microbicide to minimise the risk of intraocular infection.
- For the intravitreal injection, a **30 G x ½ inch injection needle** should be used. Use of a smaller size injection needle (higher gauge) than the 30G x 1/2 inch needle may result in increased injection forces.

- **EYLEA 40 mg/ml pre-filled syringe (2 mg dose):**
 - Expel excess volume and air bubbles from the pre-filled syringe and adjust the base of the plunger dome (**NOT the tip**) to the dose line before injection
 - Push the plunger slowly and with constant pressure, and do not administer any residual volume remaining in the syringe after injection

✓ **Correct** plunger position



- **EYLEA 114.3 mg/ml pre-filled syringe (8 mg dose):**
 - The EYLEA 114.3 mg/ml pre-filled syringe has a push and twist priming mechanism and is different from other pre-filled syringes including the EYLEA 40 mg/ml pre-filled syringe.
 - This pre-filled syringe does not have a dose line because it is designed to set the dose using the following steps:
 - Expel excess volume and air bubbles by pushing the plunger slowly and with constant pressure until it stops, i.e., when the guide on the plunger rod reaches the finger grip.
 - Turn the end of the plunger rod 90 degrees clockwise or counter-clockwise until the guide of the plunger rod aligns with the slot (click sound may be heard). Now the device is ready to be inserted into the eye for dosing.
 - Upon insertion of the needle into the injection site, inject the solution by slowly pushing the plunger rod until it stops. Do not apply additional pressure after the plunger reaches the stop.



- It is normal for a small amount of residual solution to remain in the syringe after the injection.

Selected instructions for storage and handling of EYLEA

- **Store EYLEA in the refrigerator (2°C to 8°C)**
- **Prior to use, the unopened EYLEA 40 mg/ml and 114.3 mg/ml vials and the EYLEA 40 mg/ml and 114.3 mg/ml pre-filled syringes may be kept in their cartons at room temperature (below 25°C) for up to 24 hours.**
- EYLEA is **not licensed for multi-dose**, further compounding or vial splitting. Use of more than one injection from the vial or the pre-filled syringe **can lead to contamination and subsequent infection**

GENERAL INFORMATION FOR ADULT PATIENTS

You must explain to the patient the implications of anti-VEGF treatment. The patient guide is a tool that will help you to communicate to your adult patient about the disease and treatment. This guide is available upon request to Bayer, and you should distribute it to your adult patients. It is available as a booklet and as an audio guide option for your adult patients. It contains information on the signs and symptoms of adverse reactions and when they should seek medical attention.

The Summary of Product Characteristics, or SmPC, describes the properties of EYLEA and the approved indications for use. It is an important source of information for healthcare professionals on how to use EYLEA safely and effectively. It is located at <https://www.ema.europa.eu/en/documents/product-information/eylea-epar-product->

information_en.pdf. Refer to the approved SmPC for EYLEA for complete information on posology and dosing recommendations for EYLEA 40 mg/ml solution for injection (2 mg dose) and Eylea 114.3 mg/ml solution for injection (8 mg dose).

KEY SUMMARY FOR EYLEA USE IN RETINOPATHY OF PREMATURITY

Indication in preterm infants

- Retinopathy of Prematurity (ROP) with zone I (stage 1+, 2+, 3 or 3+), zone II (stage 2+ or 3+) or AP-ROP (aggressive posterior ROP) disease.

Contraindications

- Hypersensitivity to aflibercept or to any of the excipients listed in section 6.1 of the Summary of Product Characteristics (SmPC)
- Active or suspected ocular or periocular infection
- Active severe intraocular inflammation

Key instructions for use in ROP

- **The EYLEA 2 mg pre-filled syringe is used for the treatment of preterm infants with ROP, and it must be used in combination with the PICLEO® paediatric dosing device and a low dead space 30G ½ inch (13 mm) injection needle to ensure administration of the recommended dose. Air bubbles must be removed from the syringe and device and the system must be primed. Do not use the EYLEA 8 mg pre-filled syringe for the treatment of preterm infants with ROP.**



- Ensure that the procedure is carried out in a sterile environment and that proper aseptic technique is followed, including use of a broad-spectrum microbicide to minimise risk of intraocular infection. Ensure that the injection needle is inserted into the patient's eye such that damage to the lens and the retina is avoided. Refer to the instructions for use section in this guide.
- The EYLEA 2 mg pre-filled syringe is for single use in one eye only.
- The PICLEO paediatric dosing device is for single use in one eye only.
- For the intravitreal injection, **a low dead space 30G injection needle, ½ inch (13 mm) in length** must be used. A low dead space needle has a reduced excessive space in the needle hub. **The EYLEA 2 mg pre-filled syringe contains more than the recommended dose of 0.4 mg (equivalent to 0.01 mL dose of EYLEA). Do not inject the entire volume contained in the syringe.**
- **Carefully read the Instructions for Use included in the package of the PICLEO paediatric dosing device, including the Important Information section. Also read the sections in this prescriber guide for instructions on proper storage, handling and use.**

Selected instructions for storage and handling of EYLEA

- **Store EYLEA in the refrigerator (2°C to 8°C)**; it may be kept at room temperature (below 25°C) in the unopened blister in the carton for up to 24 hours.
- EYLEA is **not licensed for multi-dose**, further compounding or splitting. Use of more than one injection from the pre-filled syringe **can lead to contamination and subsequent infection**.

Dosing recommendations for retinopathy of prematurity:

The recommended dose for EYLEA for the treatment of ROP is 0.4 mg aflibercept, equivalent to 0.01 mL. **Note that the recommended dose for the treatment of ROP patients is lower than the dose used to treat adult patients for other approved EYLEA indications.** For this reason the PICLEO paediatric dosing device must be used with the EYLEA pre-filled syringe and a low dead space needle to ensure administration of the correct dose to the patient. A low dead space needle has a reduced excessive space in the needle hub.

GENERAL INFORMATION FOR PARENT/CAREGIVER

You must explain to the parent/caregiver of your patient the implications of anti-VEGF treatment. This includes the signs and symptoms of adverse events and when the parent/caregiver of the patient should seek immediate medical attention for the patient. Please provide the EYLEA Patient Information Leaflet to the patient's parent/caregiver (which is also available on https://www.ema.europa.eu/en/documents/product-information/eylea-epar-product-information_en.pdf).

IMPORTANT SAFETY INFORMATION ABOUT EYLEA

Special warnings and precautions for use

Intravitreal injection-related reactions

Intravitreal injections, including those with EYLEA, have been associated with endophthalmitis, intraocular inflammation, rhegmatogenous retinal detachment, retinal tear and iatrogenic traumatic cataract.

- **Always use proper aseptic injection techniques** when administering EYLEA
- **Monitor patients following injections as per local practice** to permit early treatment if an infection occurs
- **Instruct adult patients to immediately report any signs and symptoms** suggestive of endophthalmitis or any of the adverse reactions mentioned below
- **In ROP, closely observe your patients for any signs and symptoms** suggestive of endophthalmitis or any of the adverse reactions mentioned below. Instruct the parent/caregiver to also closely observe the patient for the signs and symptoms noted below, and to report without delay
- **In ROP, observe your patients for any signs or symptoms of intraocular inflammation** (e.g., redness/irritation of the eye, ocular discharge, lid swelling, photophobia) that may be attributable to infection. Instruct the parent/caregiver to also observe for these signs and symptoms and to report without delay

- Refer to the post injection care section for further instructions
- **For the treatment of ROP in preterm infants, the pre-filled syringe contains more than the recommended dose of 0.4 mg aflibercept (equivalent to 0.01 mL). When treating ROP in preterm infants, the pre-filled syringe must be used in combination with the PICLEO paediatric dosing device and a low dead space needle to avoid administration of a higher than recommended volume that could result in increased intraocular pressure.**

Carefully read the instructions for use (IFU) included in the package of the PICLEO paediatric dosing device.



Increase in intraocular pressure

Transient increases in intraocular pressure have been seen within 60 minutes of intravitreal injection, including injections with EYLEA.

- **Monitor the adult patient after the injection procedure** and take special precaution in patients with poorly controlled glaucoma. Do not inject EYLEA while the intraocular pressure is ≥ 30 mm Hg. Both the intraocular pressure and perfusion status of the optic nerve head must be monitored and managed appropriately.
- **For ROP, immediately following the intravitreal injection, monitor the preterm infant for elevation in intraocular pressure and have sterile equipment available in case a paracentesis is required**
- Refer to the post-injection care section for further instructions

In all adult cases, instruct patients to immediately report signs and symptoms of adverse events

Adverse event/risk	Measures to minimise risk
Intraocular inflammation including endophthalmitis	Use proper aseptic technique when preparing the injection and during the injection itself Use recommended antiseptic agents Monitor patient after the injection
Transient IOP* increase	Properly prime the syringe by removing excess volume and air bubbles from the syringe before administration Monitor patient's vision and IOP after the injection
Medication error	Check the carton and the label on the medication to ensure you have the correct dose of Eylea.
Retinal pigment epithelial tear	Review PED features for risk of RPE tears. Monitor patient after the injection for symptoms such as acute decrease in (central) vision, blind spot (central scotoma), and distorted vision with deviation of either vertical or horizontal lines (metamorphopsia).
Cataract	Measure the correct site for the injection, use correct injection technique
Off-label use/misuse	Use medication only for treatment of approved indications, and use approved dose

Embryo-foetotoxicity	Instruct women of childbearing potential to use effective contraception during treatment: <ul style="list-style-type: none"> - For at least 3 months after last intravitreal injection of EYLEA 40 mg/ml (2 mg dose) - For at least 4 months after last intravitreal injection of EYLEA 114.3 mg/ml (8 mg dose) EYLEA 40 mg/ml (2 mg dose) and EYLEA 114.3 mg/ml (8 mg dose) should not be used during pregnancy unless the potential benefit outweighs the potential risk to the foetus
Exposure during breast-feeding	EYLEA is not recommended in patients who are breast-feeding

*Intraocular pressure

In all ROP cases, observe your patients immediately for any signs and symptoms of adverse reactions, and instruct the parent/caregiver to also be watchful for the signs and report without delay.

Adverse reaction/risk	Measures to minimise risk
Intraocular inflammation including endophthalmitis	Use proper aseptic technique when preparing the injection and during the injection itself. Use recommended antiseptic agents such as antibiotic ointment and/or drops. Monitor patients frequently post-injection and instruct the parent/caregiver to also monitor.
Transient IOP increase	The EYLEA 2 mg pre-filled syringe must be used in combination with the PICLEO paediatric dosing device, for the treatment of ROP in preterm infants. Monitor IOP and optic nerve perfusion immediately after the injection.
Medication error	The EYLEA 2 mg pre-filled syringe must be used in combination with the PICLEO paediatric dosing device, for the treatment of ROP in preterm infants. Air bubbles must be removed before use from the PICLEO paediatric dosing device + EYLEA 2 mg pre-filled syringe + low dead space 30G ½ inch (13 mm) injection needle assembly to avoid the possibility of underdosing.
Cataract	Measure for correct site of injection, use correct injection technique.
Off-label use/misuse	Use EYLEA 2 mg pre-filled syringe only in combination with the PICLEO paediatric dosing device and a low dead space injection needle for treatment of retinopathy of prematurity. Use medication only for treatment of retinopathy of prematurity and use approved dose (0.4 mg, equivalent to 0.01 mL).

Adverse drug reactions

The safety profiles observed in the clinical program for EYLEA 40 mg/ml (2 mg dose) and EYLEA 114.3 mg/ml (8 mg dose) in adult indications are similar. See section 4.8 of the respective SmPCs for full list of potential adverse reactions and their frequency categories.

In ROP, adverse reactions reported in more than one patient treated with aflibercept 0.4 mg were retinal detachment, conjunctival haemorrhage, injection site haemorrhage, intraocular pressure increased, eyelid oedema and retinal haemorrhage. Additionally, adverse reactions established for adult indications are considered applicable to pre-term infants with ROP, though not all were observed in the phase III paediatric study.

Key signs and symptoms of intravitreal injection-related adverse reactions include:

Adverse Drug Reaction	Key signs and symptoms
Transient increased intraocular pressure	<p>Adult patients may experience vision changes such as temporary vision loss, eye pain, halos around lights, red eye, nausea and vomiting.</p> <p>Preterm infant may experience cloudy anterior segment of eyeball (corneal oedema), rock-hard eyeball, red eye, paroxysmal crying, nausea and vomiting.</p>
Tear of the retinal pigment epithelium	<p>Adult patients may experience acute decrease in (central) vision, blind spot (central scotoma), and distorted vision with deviation of either vertical or horizontal lines (metamorphopsia)</p>
Tear or detachment of the retina	<p>Adult patients may experience sudden flashes of light, a sudden appearance or an increase of the number of vitreous floaters, a curtain over a portion of their visual field and vision changes.</p> <p>Preterm infant may experience white pupil (leukocoria), newly observed crossed eyes (strabismus) and vision changes.</p>
Intraocular inflammation including endophthalmitis	<p>Adult patients may experience eye pain or increased discomfort, worsening eye redness, photophobia or sensitivity to light, swelling, and vision changes, such as a sudden decrease in vision or blurring of vision.</p> <p>Preterm infant may experience eye pain or increased discomfort, worsening eye redness, sensitivity to light (photophobia), lid swelling, paroxysmal crying and ocular discharge.</p>
Cataract (traumatic, nuclear, subcapsular, cortical) or lenticular opacities	<p>Adult patients may experience less vivid lines and shapes, shadows and colour vision than before, and vision changes.</p>
Cataract (traumatic)	<p>Preterm infant may experience white pupil, loss of red reflex and vision changes.</p>

See section 4.8 of the SmPC for the full list of potential adverse reactions.

Post-Injection care in Adults

Immediately after intravitreal injection:

- Evaluate the patient's vision (hand movement or finger counting).
- Monitor the patient for elevation in intraocular pressure. Appropriate monitoring may consist of a check for perfusion of the optic nerve head or conducting a tonometry test. Sterile equipment for paracentesis should be readily available if anterior chamber paracentesis needs to be done.
- Instruct the patient to report any signs and symptoms suggestive of endophthalmitis (e.g. eye pain, redness of the eye, photophobia, blurring of vision) without delay.
- Instruct the patient to report any signs or symptoms after the injection that get worse over time.

Post-Injection care in ROP

Immediately after intravitreal injection:

- Immediately monitor the patient for elevation in intraocular pressure. Appropriate monitoring may consist of fundus examination including a check for perfusion of the central retinal artery, or conducting a tonometry test. Sterile equipment for paracentesis should be readily available if anterior chamber paracentesis needs to be done.

After intravitreal injection:

- Observe your patient for any signs and symptoms suggestive of endophthalmitis (e.g., redness of the eye, photophobia, irritation of the eye, ocular discharge, lid swelling) without delay.
- Observe your patient for any signs or symptoms after the injection that get worse over time and instruct the parent/caregiver to do the same, and to report any observed signs and symptoms without delay.

Management of adverse reactions

In case of any adverse reactions that concern your patient, they must have immediate access to an ophthalmologist.

Appropriate management of ALL adverse reactions, including those associated with the intravitreal injection, should be carried out according to clinical practice and/or following standardised guidelines.

Healthcare Professionals are asked to report any suspected adverse reactions. See section 4.8 of the SmPC for how to report suspected adverse reactions.

Risk of medication error when used in adults

Eylea is available as a 40 mg/ml (2 mg dose) pre-filled syringe or vial and a 114.3 mg/ml (8 mg dose) pre-filled syringe or vial. The approved indications, dose and posology differ between the 40 mg/ml strength and the 114.3 mg/ml strength. Please refer to the table on the 'Differences between EYLEA 40 mg/ml solution for injection (2 mg dose) and EYLEA 114.3 mg/ml solution for injection (8 mg dose)', the Storage and Handling of EYLEA and Section 4.2 and Section 6.6 of the SmPC to differentiate the product to be injected into the patient. The EYLEA 40 mg/ml vial and pre-filled syringe are different from the EYLEA 114.3 mg/ml vial and pre-filled syringe, including in their appearance, to allow easy identification.

In both EYLEA 40 mg/ml solution for injection (2 mg dose) and EYLEA 114.3 mg/ml solution for injection (8 mg dose), the pre-filled syringe and the vial contain more than the adult recommended dose of 2 mg or 8 mg aflibercept (equivalent to 0.05 ml/0.07ml).

Expel the excess volume, to avoid overdosing, and air bubbles from the syringe prior to injection. The EYLEA 114.3 mg/ml pre-filled syringe has a push and twist priming mechanism and is different from other pre-filled syringes including the EYLEA 40 mg/ml pre-filled syringe.

Pregnancy and breast-feeding in adults

The following recommendations are made:

- **Women of childbearing potential**
Use effective contraception during treatment and for at least 3 months after the last intravitreal injection of EYLEA 40 mg/ml (2 mg dose).
Use effective contraception during treatment and for at least 4 months after the last intravitreal injection of EYLEA 114.3 mg/ml (8 mg dose).
- **Pregnancy**
There are no data on the use of aflibercept in pregnant women. Studies in animals have shown embryo-foetal toxicity.
EYLEA 2 mg and EYLEA 8 mg should not be used during pregnancy unless the potential benefit outweighs the potential risk to the foetus.
- **Breast-feeding**
Based on very limited human data, aflibercept may be excreted in human milk at low levels. Aflibercept is a large protein molecule and the amount of medication absorbed by the infant is expected to be minimal. The effects of aflibercept on a breast-fed newborn/infant is unknown. As a precautionary measure, breast-feeding is not recommended during the use of Eylea.

STORAGE AND HANDLING OF EYLEA

The EYLEA 40 mg/ml (2 mg dose) solution is clear and the EYLEA 114.3 mg/ml (8 mg dose) solution is clear to slightly opalescent. Both solutions are colourless to pale yellow. It is an iso-osmotic solution.

Inspect the solution visually before use, for any foreign particulate matter and/or unusual colour (the solution can be pale yellow, which is normal) **or any variation in physical appearance. If any of these are observed, do not use the product.**

The EYLEA 40 mg/ml vial and pre-filled syringe are different from the EYLEA 114.3 mg/ml vial and pre-filled syringe, including in their appearance, to allow easy identification. Please take this into consideration when selecting the product to be administered (please see pictures below).

Inspect the pre-filled syringe. If any part is damaged or loose, or if the syringe cap is detached from the Luer Lock, do not use.

Do not split a vial/pre-filled syringe into more than one dose. Each vial/pre-filled syringe is for single use in one eye only. Extraction of multiple doses from a single vial/pre-filled syringe may increase the risk of contamination and subsequent infection in the patient.

Eylea 40 mg/ml pre-filled syringe and vial for use in adults:



Each EYLEA 40 mg/ml solution for injection in a pre-filled syringe (2 mg dose) contains **more than the recommended 0.05 ml dose of aflibercept.**

Correct handling of the pre-filled syringe is important in order to avoid the risk of medication errors. This includes removal of the excess volume (to avoid overdosing) and air bubbles from the syringe, prior to injection.



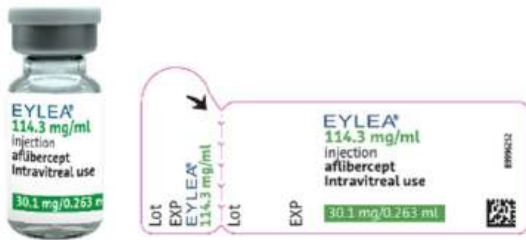
Each EYLEA 40 mg/ml solution for injection in a vial (2 mg dose) **contains more than the recommended 0.05 mL dose of aflibercept.**

Correct handling of the filled syringe is important in order to avoid the risk of medication errors. This includes removal of the excess volume (to avoid overdosing) and air bubbles from the disposable syringe, prior to injection.

Eylea 114.3 mg/ml pre-filled syringe and vial for use in adults:



Each EYLEA 114.3 mg/ml solution for injection in a pre-filled syringe (8 mg dose) contains more than the recommended 0.07 ml dose of aflibercept. The excess volume and any air bubbles in the syringe must be expelled before injecting according to the priming steps in the instructions for use. **Remember that the priming steps of this syringe differ from other pre-filled syringes. Carefully review the instructions below.**



Each EYLEA 114.3 mg/ml solution for injection in a vial (8 mg dose) **contains more than the recommended 0.07 ml dose of EYLEA.** Correct handling of the filled syringe is important in order to avoid the risk of medication errors. This includes removal of the excess volume (to avoid overdosing) and air bubbles from the disposable syringe, prior to injection.

Eylea 40 mg/ml pre-filled syringe and PICLEO paediatric dosing device for use in ROP







Each pre-filled syringe contains more than the recommended dose of 0.4 mg EYLEA (equivalent to 0.01 mL)



To ensure the administration of the recommended dose, the pre-filled syringe must be used with the PICLEO paediatric dosing device and a low dead space 30G 1/2 inch (13 mm) needle. Please refer to the section “Important information about the PICLEO paediatric dosing device” in this guide

Special precautions for storage of the EYLEA vial and pre-filled syringe

	<p>Store the pre-filled syringe in the sealed blister in the outer carton in a refrigerator (2–8°C).</p> <p>Store the vial in a refrigerator (2–8°C).</p>
	<p>Prior to use, the unopened EYLEA 40 mg/ml and EYLEA 114.3 mg/ml vials and the unopened EYLEA 40 mg/ml and EYLEA 114.3 mg/ml pre-filled syringe blisters may be kept in their cartons at room temperature (below 25°C) for up to 24 hours.</p>
	<p>Do not freeze.</p>
	<p>Keep the pre-filled syringe in its blister and in the outer carton in order to protect it from light.</p> <p>Keep the vial in the outer carton in order to protect from light.</p>

The inside of the sealed pre-filled syringe blister packaging, and the pre-filled syringe itself of EYLEA 40 mg/ml (2 mg dose) and EYLEA 114.3 mg/ml (8 mg dose) solution for injection are sterile. Do not open the pre-filled syringe blister outside the clean administration room.

After opening the blister or vial, proceed under aseptic conditions.

Storage and handling instructions for the PICLEO paediatric dosing device



Carefully read the instructions for use (IFU) included in the package of the PICLEO paediatric dosing device.

Do not use the PICLEO device for more than one dose. The PICLEO paediatric dosing device is for single use in one eye only. Never re-use the device as it will malfunction, and contamination increases the risk to the patient of intraocular infection.

It is recommended to store the PICLEO paediatric dosing device at room temperature.

Keep it within its original packaging. Keep it away from sunlight.

Do not open the sealed blister pack before time of use. Do not use beyond the use-by date.



The inside of the blister of the sealed PICLEO paediatric dosing device packaging and the PICLEO paediatric dosing device itself are sterile. Do not open the PICLEO paediatric dosing device blister outside the clean administration room. After opening the blister, proceed under aseptic conditions.

INSTRUCTIONS FOR USE OF EYLEA IN ADULTS

General preparation for injection

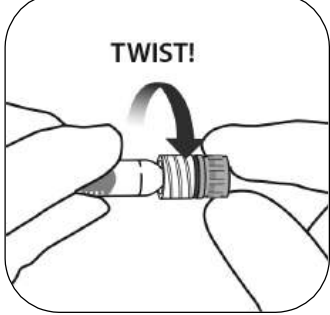
- Intravitreal injections must be carried out according to medical standards and applicable guidelines by **a qualified physician experienced in administering intravitreal injections and familiar with the handling** of the vial/pre-filled syringe.
- Surgical hand disinfection, aseptic gloves, a sterile drape and a sterilised eyelid speculum (or equivalent) are recommended.
- For the intravitreal injection, a **30 G x ½ inch injection needle** should be used. Use of a smaller size injection needle (higher gauge) than the 30G x 1/2 inch needle may result in increased injection forces.


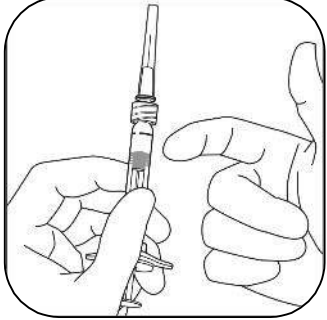

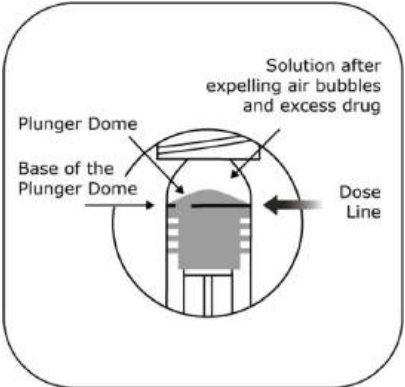

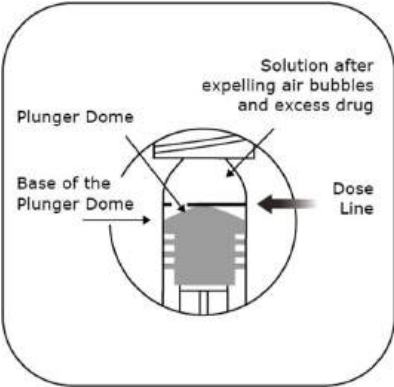
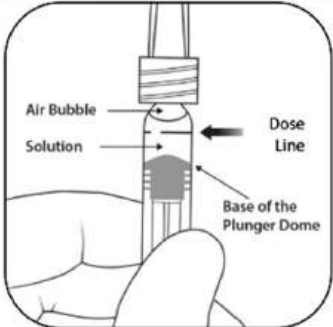
Pre-filled syringe 40 mg/ml (2 mg dose), solution for injection (for use in adults)

Note: Become familiarised with how to use this syringe before using it on patients.

The EYLEA 40 mg/ml pre-filled syringe is a glass syringe with a rubber plunger that requires slightly more force to depress compared with plastic syringes (such as those used with the vial presentation).

The pre-filled syringe and contents must be inspected before use. Do not use the pre-filled syringe if any part is damaged or loose. Do not use it if the syringe cap is detached from the Luer Lock. Look for any particulate matter and/or unusual colour or any variation in physical appearance. If any of these are observed, do not use the product.

1	<p><u>Prepare the pre-filled syringe for administration</u> It is important to prepare the pre-filled syringe using aseptic technique.</p> <p>An assistant should carry out the following steps: Remove the carton containing the pre-filled syringe from the refrigerator. Open the carton and remove the blister containing the syringe. The blister must not be placed on an aseptic surface because the outside surface of the blister is not sterile. The inside of the sealed blister and the pre-filled syringe are sterile. Carefully peel open the blister. Aseptic technique must be used once the blister is opened.</p> <p>The qualified physician carries out the remainder of the steps with sterile technique including the use of aseptic gloves (white gloves in pictures) when handling: With two fingers, remove the pre-filled syringe from the blister. Visually inspect the syringe. Place the syringe in a sterile tray until ready for assembly.</p>
2	<p><u>Remove the syringe cap</u> Hold the syringe in one hand while using the other hand to grasp the syringe cap with the thumb and forefinger. Twist off – do not snap off – the syringe cap.</p> 

3	<p>Do not pull back the plunger. This may compromise the sterility of the product.</p>
4	<p><u>Attach the needle</u> Using aseptic technique, firmly twist the 30 G x ½ inch injection needle onto the Luer-lock syringe tip.</p> 
5	<p><u>Check for bubbles</u> Holding the syringe with the needle pointing upwards, check the solution for bubbles. If bubbles are present, gently tap the syringe with your finger until the bubbles rise to the top.</p> 
6	<p><u>Eliminate air bubbles and excess drug</u> Correct handling of the pre-filled syringe is important in order to avoid the risk of medication errors. This includes removal of the excess volume (to avoid overdosing) and air bubbles.</p> <p>Remove the air bubbles and excess drug from the syringe by slowly depressing the plunger rod to align the base of the plunger dome (not the tip of the dome) with the dose line on the syringe. Remember that the feel with this syringe is different from disposable syringes. The remaining volume after aligning to the dose line ensures an injection volume of 0.05 mL.</p> <p>Accurate positioning of the plunger is critical. Incorrect plunger positioning can lead to delivering more or less than the labelled dose.</p> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="text-align: center;">  <p>Correct plunger position</p>  </div> <div style="text-align: center;">  <p>Incorrect plunger position</p>  </div> </div> 

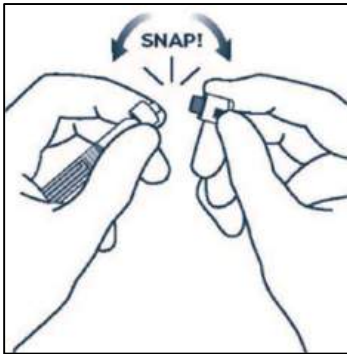
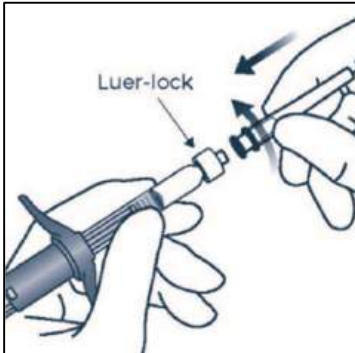
7	<p><u>Inject EYLEA</u></p> <p>Inject the solution into the eye carefully with constant pressure on the plunger. Do not apply additional pressure once the plunger has reached the bottom of the syringe.</p> <p>Do not administer any residual solution observed in the syringe.</p>
8	<p>The pre-filled syringe is for single use only.</p> <p>Dispose of any unused medicinal product or waste material in accordance with local regulations.</p>


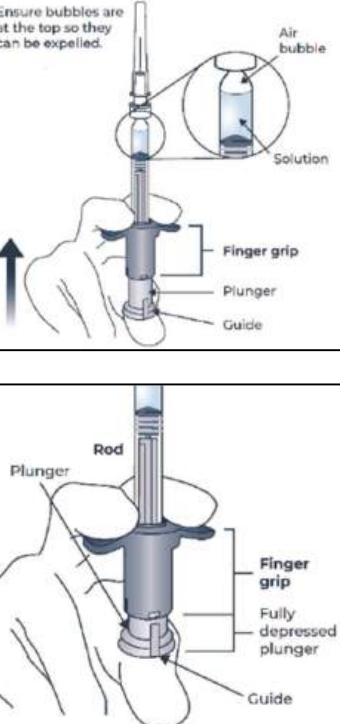
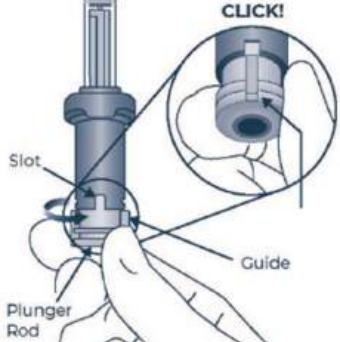
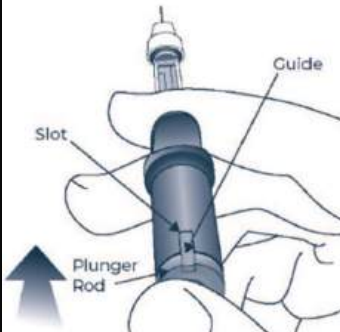
Pre-filled syringe 114.3 mg/ml (8 mg dose), solution for injection (for use in adults)

Note: Become familiarized with how to use this syringe before using it on patients.


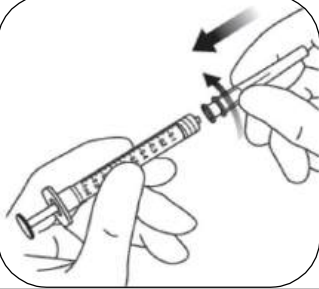

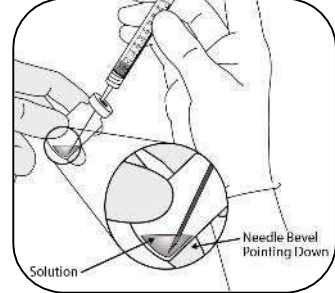
The EYLEA 114.3 mg/ml pre-filled glass syringe does not have a dose line because it is designed to set the dose using the steps listed below. Residual solution will remain in the syringe after the injection, and is to be discarded.

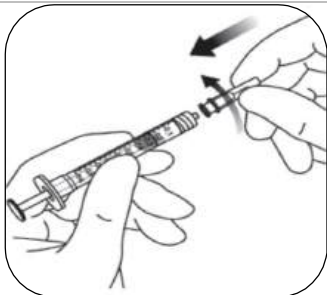
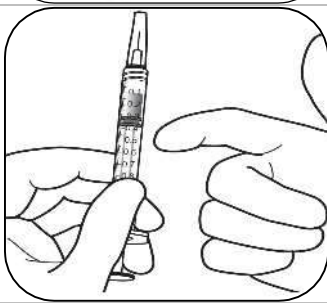
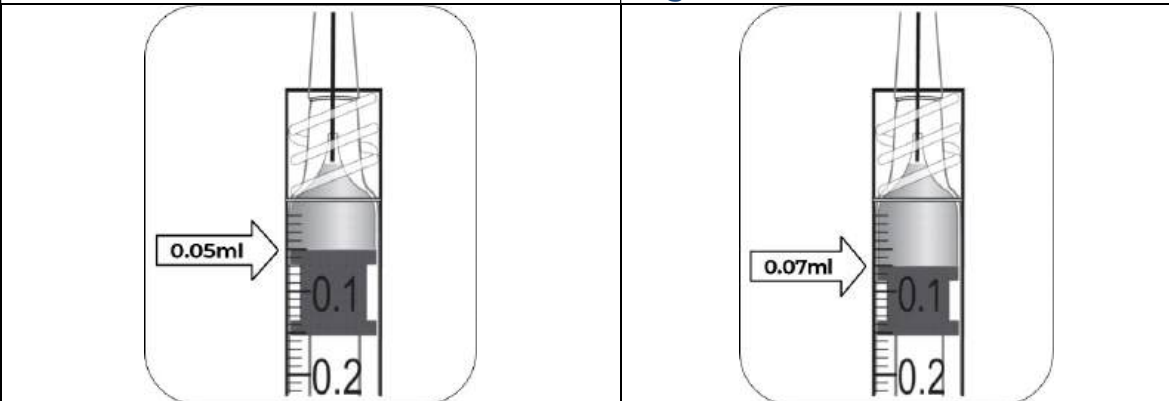
The pre-filled syringe and contents must be inspected before use. Do not use the pre-filled syringe if any part is damaged or loose. Do not use it if the syringe cap is loose or detached from the syringe. Look for any particulate matter and/or unusual colour or any variation in physical appearance. If any of these are observed, do not use the product.

1	<p><u>Prepare the pre-filled syringe for administration</u></p> <p>It is important to prepare the pre-filled syringe using aseptic technique. An assistant should carry out the following steps: Remove the carton containing the pre-filled syringe from the refrigerator. Open the carton and remove the blister containing the syringe. The blister must not be placed on an aseptic surface because the outside surface of the blister is not sterile. The inside of the sealed blister and the pre-filled syringe are sterile. Carefully peel open the blister. Aseptic technique must be used once the blister is opened.</p> <p>The remaining steps have to be carried out by a qualified physician using aseptic technique including the use of sterile gloves (white gloves in pictures) when handling.</p> <p>With two fingers, remove the pre-filled syringe from the blister, visually inspect the syringe and place the syringe in a sterile tray until ready for assembly.</p>
2	<p>SNAP OFF (do not twist off) syringe cap by holding the syringe in one hand and the syringe cap with the thumb and forefinger of the other hand</p> <p>Note: Do not pull back on the plunger rod.</p> 
3	<p><u>Attach needle</u></p> <p>Firmly twist the 30G x ½ inch injection needle onto the Luer-lock syringe tip.</p> <p>Use of a smaller size injection needle (higher gauge) than the 30G x ½ inch needle may result in increased injection forces.</p> 

4	<p><u>Dislodge air bubbles</u></p> <p>Holding the syringe with the needle pointing up, check the syringe for bubbles. If there are bubbles, gently tap the syringe with your finger until the bubbles rise to the top.</p>	
5	<p><u>Expel air and excess volume to prime</u></p> <p>The Eylea 114.3 mg/ml pre-filled syringe does not have a dose line because it is designed to set the dose mechanically. Priming and setting the dose must be done using the following steps. To eliminate all bubbles and to expel excess drug, slowly depress the plunger rod (top figure) until it stops, i.e. when the guide on the plunger rod reaches the finger grip (bottom figure).</p>	
6	<p><u>Set to dose</u></p> <p>Turn the end of the plunger rod 90 degrees clockwise or counterclockwise until the guide of the plunger rod aligns with the slot. You may hear a “click”.</p> <p>Note: Now the device is ready to dose. Do not push the plunger rod before insertion into the eye.</p>	
7	<p><u>Administer the injection</u></p> <p>Insert the needle into the ocular injection site. Inject the solution by pushing in the plunger rod until it stops, i.e. until the guide is completely within the slot. Do not apply additional pressure once the guide is within the slot. It is normal to see a small amount of residual solution left in the syringe.</p>	
8	<p>The pre-filled syringe is for single use only.</p> <p>Dispose of any unused medicinal product or waste material in accordance with local regulations.</p>	




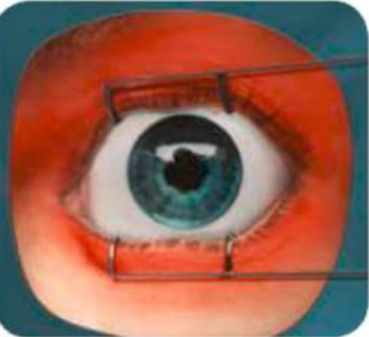
Vial 40 mg/ml (2 mg dose) and 114.3 mg/ml (8 mg dose) solution for injection (for use in adults)

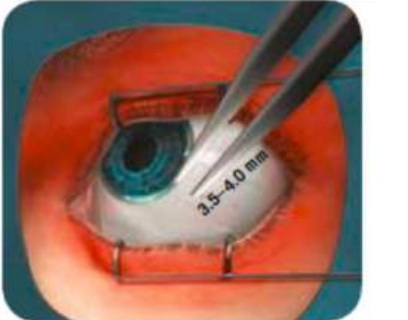
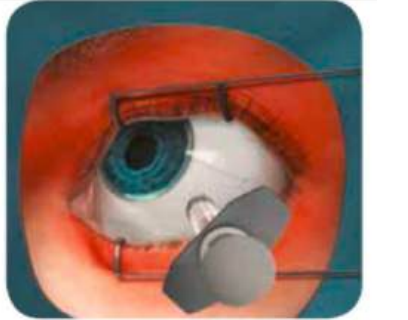
<p>1</p>	<p><u>Inspect the vial, and remove the vial cap</u></p> <p>It is important to prepare the syringe with EYLEA from the vial, using aseptic technique. Note in the pictures that darker/grey gloves are not aseptic and white gloves are aseptic.</p> <p>An assistant should carry out the following steps (assistant is shown with darker gloves in the images): Remove the carton containing the vial from the refrigerator. Let the carton and its contents reach room temperature. Open the carton, remove the vial and place it upright on a flat surface to allow the solution to accumulate at the bottom of the vial.</p> <p>Check the carton, the vial and label to ensure the correct EYLEA solution is chosen. The vial should not be placed on an aseptic surface because the outside surface of the vial is not sterile. The inside of the vial is sterile.</p> <p>Check that the liquid is at the bottom of the vial. Visually inspect the vial and contents (the liquid). Remove the plastic cap and disinfect the outer part of the rubber vial stopper.</p>	
<p>2</p>	<p><u>Attach the filter needle</u></p> <p>The qualified physician should carry out the remaining steps using aseptic technique, including the use of aseptic gloves: Using aseptic technique, screw on the 18 G, 5-micron filter needle supplied in the carton to a 1 mL sterile Luer-lock syringe.</p>	
<p>3</p>	<p><u>Insert needle into vial</u></p> <p>Insert the filter needle into the centre of the vial stopper until the needle is completely inserted into the vial and the needle tip touches the bottom or bottom edge of the vial.</p>	
<p>4</p>	<p><u>Draw up the solution</u></p> <p>Withdraw all of the EYLEA vial contents slowly into the syringe, keeping the vial in an upright position, slightly inclined to ease complete withdrawal. This helps to prevent air bubbles. To avoid the introduction of air, ensure the bevel of the filter needle is submerged in the liquid. Continue to tilt the vial while withdrawing to allow the liquid to collect to the corner of the vial, keeping the bevel of the filter needle submerged in the liquid.</p> <p>Ensure that the plunger rod is drawn sufficiently back when emptying the vial in order to completely empty the filter needle.</p>	

5	<p><u>Remove the filter needle</u> Unscrew and properly dispose of the filter needle. Do not use the filter needle for intravitreal injection.</p>							
6	<p><u>Attach the injection needle</u> Using aseptic technique, firmly twist a 30G x ½ inch injection needle to the Luer-lock syringe tip. Use of a smaller size injection needle (higher gauge) than the 30G x ½ inch needle may result in increased injection forces.</p>							
7	<p><u>Check for air bubbles</u> Holding the syringe with the needle pointing upwards, visually inspect the contents of the syringe. Check the solution for bubbles. If bubbles are present, gently tap the syringe with your finger until the bubbles rise to the top.</p>							
8	<p><u>Eliminate air bubbles and excess drug</u> Correct handling of the filled syringe is important in order to avoid the risk of medication errors. This includes removal of the excess volume (to avoid overdosing) and air bubbles.</p> <p>Attention! The EYLEA 2 mg dose uses 0.05 ml volume of EYLEA 40 mg/ml solution. The EYLEA 8 mg dose uses 0.07 ml volume of EYLEA 114.3 mg/ml solution.</p> <table border="1" data-bbox="236 1153 1410 1478"> <thead> <tr> <th data-bbox="236 1153 858 1189">EYLEA 2 mg dose</th> <th data-bbox="858 1153 1410 1189">EYLEA 8 mg dose</th> </tr> </thead> <tbody> <tr> <td data-bbox="236 1189 858 1263">Use 0.05 ml volume of EYLEA 40 mg/ml solution</td> <td data-bbox="858 1189 1410 1263">Use 0.07 ml of EYLEA 114.3 mg/ml solution</td> </tr> <tr> <td data-bbox="236 1263 858 1478">Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.05 ml line on the syringe for the EYLEA 40 mg/ml vial.</td> <td data-bbox="858 1263 1410 1478">Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.07 ml line on the syringe for the EYLEA 114.3 mg/ml vial.</td> </tr> </tbody> </table> <div data-bbox="236 1478 1410 1877">  </div> <p>Accurate positioning of the plunger shown in the diagrams above is critical. Incorrect plunger positioning can lead to delivering more or less than the recommended dose.</p>		EYLEA 2 mg dose	EYLEA 8 mg dose	Use 0.05 ml volume of EYLEA 40 mg/ml solution	Use 0.07 ml of EYLEA 114.3 mg/ml solution	Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.05 ml line on the syringe for the EYLEA 40 mg/ml vial.	Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.07 ml line on the syringe for the EYLEA 114.3 mg/ml vial.
EYLEA 2 mg dose	EYLEA 8 mg dose							
Use 0.05 ml volume of EYLEA 40 mg/ml solution	Use 0.07 ml of EYLEA 114.3 mg/ml solution							
Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.05 ml line on the syringe for the EYLEA 40 mg/ml vial.	Eliminate all air bubbles and expel excess drug by slowly depressing the plunger rod to align the flat plunger edge with the 0.07 ml line on the syringe for the EYLEA 114.3 mg/ml vial.							
9	<p>Each vial is for single use only. Dispose of any unused medicinal product or waste material in accordance with local regulations.</p>							

Injection Procedure for Adults

For further information on intravitreal injection procedure, sterile techniques (including periocular and ocular disinfection) and anaesthesia, please refer to local and/or national clinical guidelines.


1	Administer topical anaesthesia. Eye dilation prior to the injection procedure is not necessary.	
2	Apply disinfectant (e.g. 5% povidone iodine solution or equivalent) to the eyelids, eyelid margins and into the conjunctival sac. The disinfectant should be on the surface for at least 30 seconds. ¹	
3	A disinfectant (e.g. 10% povidone iodine solution or equivalent) should also be applied to the periocular skin, eyelids and eyelashes, avoiding extensive pressure to the periocular glands. The disinfectant should be on the surface for at least 30 seconds. ¹	
4	Cover with sterile drape and insert sterile lid speculum. A second application of disinfectant, e.g., 5% povidone iodine solution, may be made to the conjunctival sac. Disinfectant should be on the surface for at least 30 seconds. ¹	

5	<p>Tell patient to look away from the injection site. Position the eye adequately. At an area of 3.5–4.0 mm posterior to the limbus, mark an injection site.</p>	
6	<p>Insert the injection needle into the vitreous cavity, avoiding the horizontal meridian and aiming towards the centre of the globe.</p> <p>Inject the recommended dose, with careful and constant pressure on the plunger. Do not apply additional pressure once the plunger has reached the bottom of the syringe. Do not inject any residual volume remaining in the syringe after the injection.</p> <p>Use a different scleral site for subsequent injections.</p>	

1) Grzybowski, A et al. 2018 Update on intravitreal injections: EURETINA expert consensus recommendations. *Ophthalmologica*. 2018;239 (4): 181-193.

INSTRUCTIONS FOR USE OF EYLEA IN ROP

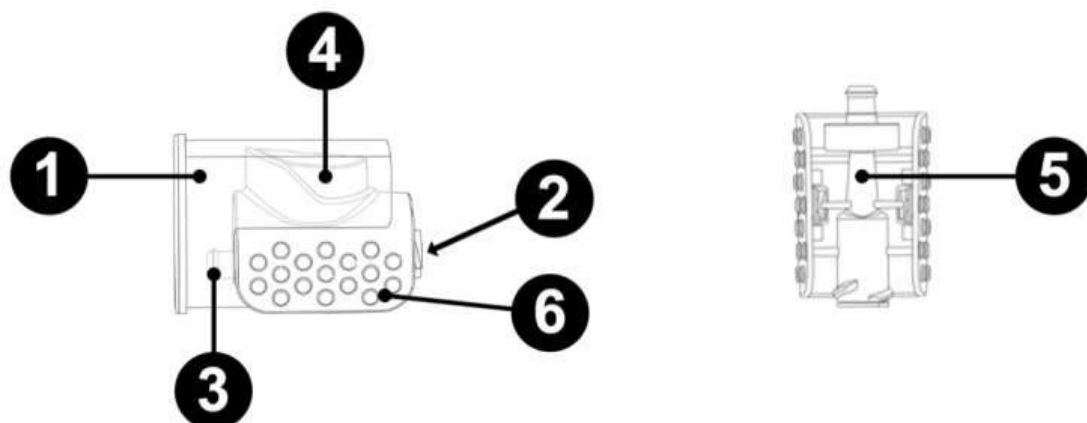
General preparation for injection

- Intravitreal injections in preterm infants must be carried out according to medical standards and applicable guidelines by a qualified physician experienced in administering intravitreal injections. **The physician must be trained to properly use the EYLEA 2 mg pre-filled syringe together with the PICLEO paediatric dosing device and low dead space injection needle. Training on assembly with the use of demonstration samples is required**
- **Ensure that you read the instructions for use provided with the PICLEO paediatric dosing device** 
- Surgical hand disinfection, sterile gloves, a sterile drape and a sterilised eyelid speculum (or equivalent) are recommended
- For the intravitreal injection, a **30 G ½ inch (13 mm) low dead space injection needle** must be used. The following injection needles are recommended:
 - TSK, 30G x ½" / 0.3 x 13 mm (Art. N. LDS-300131-100)
 - OcuJect - OcuSafe®, 30G x ½" / 0.3 x 13 mm (Art. N. PN0403-03)Any other combinations are not supported by the manufacturer of the device
- Check the expiration date of the EYLEA 2 mg pre-filled syringe and of the PICLEO paediatric dosing device. Do not use the pre-filled syringe or the paediatric dosing device if the packaging is damaged/open or if any parts of the products are broken or loose

Important information about the PICLEO paediatric dosing device

- Use the PICLEO paediatric dosing device only with the EYLEA 2 mg pre-filled syringe and a low dead space 30G ½ inch (13 mm) injection needle because it is designed for use only in combination with these two components. Use only a low dead space injection needle as use of other needles could lead to underdosing
- The PICLEO paediatric dosing device is sterile. Do not use if the packaging is damaged or has been tampered with
- Use aseptic technique when removing the PICLEO paediatric dosing device from its blister pack and for all subsequent steps to prevent contamination
- Assemble the syringe and injection needle firmly to the PICLEO paediatric dosing device to avoid leakage as well as accidental detachment
- Air bubbles must be removed from the syringe and device and the system must be primed. When using the PICLEO paediatric dosing device with the pre-filled syringe, it is not required to align the syringe plunger of the pre-filled syringe with the dosing line on the syringe when using the PICLEO paediatric dosing device
- Make sure not to touch the blue dose button of the PICLEO paediatric dosing device before the medicinal product administration. Should the dose button be inadvertently depressed during assembly, do not proceed and discard the device and the pre-filled syringe. Select a new PICLEO paediatric dosing device and follow assembly procedure steps using a new pre-filled syringe
- Medicinal product will remain in the syringe and the PICLEO paediatric dosing device after correct dose administration. Do not administer this residual solution but discard it

- The PICLEO paediatric dosing device is for single use in one eye only. Never re-use the device as it will malfunction, and contamination increases the risk of intraocular infection



1. Cover
2. Connection for the syringe (female Luer Connector)
3. Connection for the needle (male Luer Connector)
4. Dose button
5. Viewing window
6. Grip area

Pre-filled syringe (for use in ROP)

Note: the EYLEA 2 mg pre-filled syringe is a glass syringe with a rubber plunger that requires slightly more force to depress compared with plastic syringes. **Become familiar with the features of this syringe before attaching it to the PICLEO paediatric dosing device.**

Preparation of administration

1. Prepare the EYLEA 2 mg pre-filled syringe for attachment to the PICLEO paediatric dosing device

It is important to prepare the EYLEA 2 mg pre-filled syringe and the paediatric dosing device using aseptic technique.

In the figures, the assistant is shown wearing darker gloves to indicate contact to non-sterile surface.

The assistant should remove the carton containing the pre-filled syringe from the refrigerator. Note that the pre-filled syringe can be stored in the carton at room temperature for up to 24 hours. Open the carton and remove the blister containing the syringe. The blister must not be placed on a sterile surface because the outside surface of the blister is not sterile. The inside of the sealed blister and the pre-filled syringe are sterile. Carefully peel open the pre-filled syringe blister. **Aseptic technique must be used once the blister is opened.**

The assistant should open the carton of the PICLEO paediatric dosing device and remove the sealed blister pack. Carefully peel open the device blister. **Aseptic technique must be used once the blister is opened. Note: The outside of the blister pack is non-sterile. The inside of the blister pack is sterile. Do not place the blister on a sterile surface.**

The qualified physician carries out the remainder of the steps using aseptic technique including the use of sterile gloves.

2. Prepare the PICLEO paediatric dosing device for administration

With two fingers, remove the pre-filled syringe from the blister. Visually inspect the syringe for loose or damaged parts and inspect the solution in the syringe for particulate matter and discolouration. Place the syringe in a sterile tray until ready for assembly.

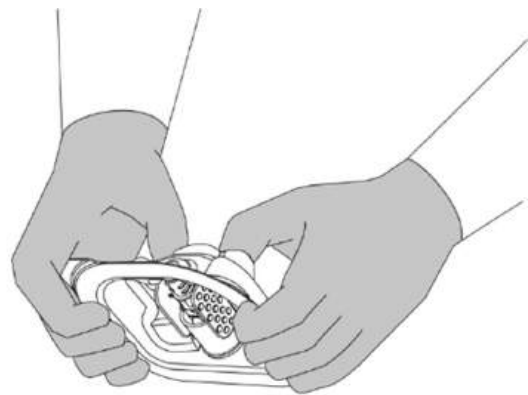
Using aseptic technique, carefully remove the PICLEO paediatric dosing device from its blister pack by taking it out with two fingers, while your assistant holds the blister from the outside, as shown in Figure a. Alternatively, your assistant can open the blister pack, and drop the PICLEO paediatric device onto a sterile surface as shown in Figure b.

Only the inside of the blister pack and the enclosed PICLEO paediatric dosing device are sterile. To avoid contamination, do not touch the Luer Connectors.

Figure a

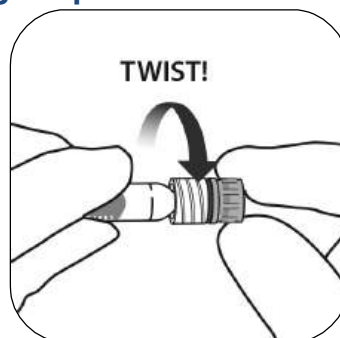


Figure b

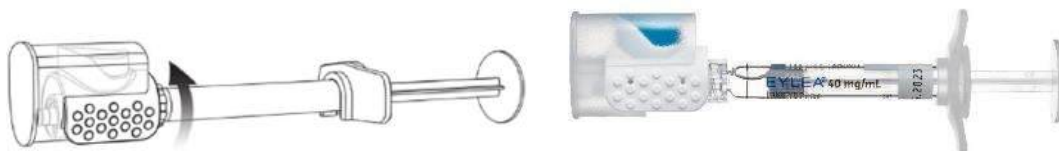


3. Attachment of the EYLEA 2 mg prefilled syringe to the device.

Remove the pre-filled syringe cap by holding the syringe in one hand while using your other hand to grasp the syringe cap with the thumb and forefinger. **Twist off – do not snap off – the syringe cap.**



Hold the PICLEO paediatric dosing device at the finger grips. Firmly twist the syringe onto the female Luer connector of the PICLEO paediatric dosing device. Make sure the connection is firm.



4. Attach the low dead space 30 G ½ inch (13 mm) injection needle to the PICLEO paediatric dosing device

Hold the Picleo paediatric dosing device at the grip area and carefully remove the cover from the PICLEO paediatric dosing device by pulling it straight off.

Do not touch the dose button when assembling. If it is pressed or partially pressed in error, it will not deliver the recommended dose. If pressed, the system needs to be discarded and you need to start again with a new device and pre-filled syringe. Do not depress the syringe plunger rod when assembling.



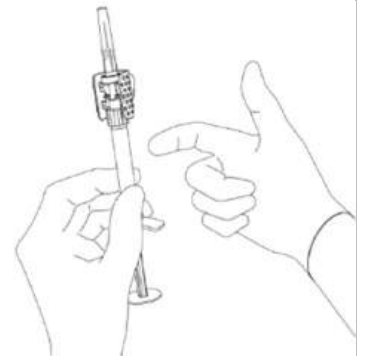
Hold the PICLEO paediatric dosing device at the grip area and firmly twist the low dead space 30 G ½ inch (13 mm) length injection needle onto the male Luer connector of the PICLEO paediatric dosing device. The device has been validated with EYLEA 2 mg pre-filled syringe and the low dead space 30G ½ inch (13 mm) injection needle only.

The EYLEA 2 mg pre-filled syringe and injection needle must be firmly attached to the PICLEO paediatric dosing device to avoid accidental detachment and to avoid leakage.



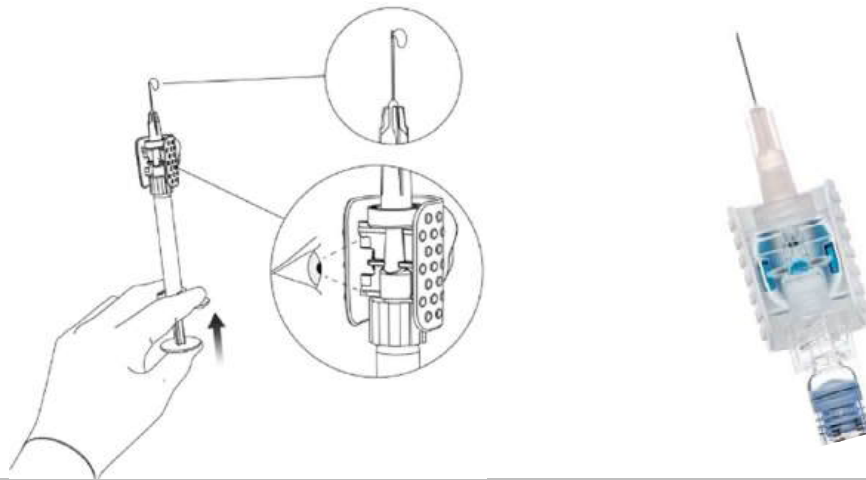
5. Inspection and priming of the system

Hold the EYLEA 2 mg pre-filled syringe with the injection needle pointing upwards and the viewing window of the PICLEO paediatric dosing device facing towards you. Inspect the medicinal product and the PICLEO paediatric dosing device for particles. Do not use if particulates are visible. Check the syringe for air bubbles. If there are any air bubbles, gently tap the syringe with your finger until the bubbles rise to the top.



Remove the cap from the needle. Prime the system by slowly depressing the plunger rod while observing through the viewing window. Eliminate air bubbles from the syringe and the PICLEO paediatric dosing device. The system is now ready for intravitreal injection.

Caution: Aligning the syringe plunger with the dosing line on the syringe is not required. After air removal and priming, the PICLEO paediatric dosing device and injection needle contain the required volume. To avoid compromising the sterility of the medicinal product, do not pull-back the plunger.




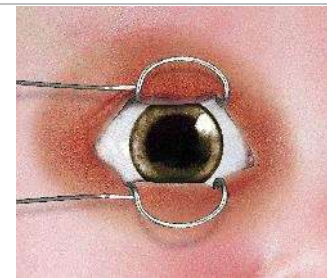
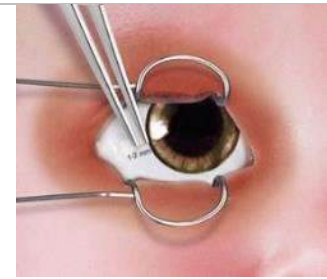


The system is now ready for intravitreal injection.

After injection, dispose of any unused medicinal product or waste material in accordance with local regulations.

Injection Procedure for ROP

For further information on intravitreal injection procedure, sterile techniques (including periocular and ocular disinfection) and anaesthesia, please refer to local and/or national clinical guidelines.

1	Administer topical anaesthesia.	
2	Apply disinfectant (e.g., povidone iodine solution or equivalent) to the periocular skin, eyelashes, eyelids, and into the conjunctival sac, avoiding extensive pressure to the periocular glands. The disinfectant should be on the surface according to local clinical guidelines.	 
3	Cover with sterile drape as needed and insert a sterile lid speculum to keep the eyelids open. Apply a second application of disinfectant (e.g., povidone iodine solution). The disinfectant should be on the ocular surface (conjunctival sac) in accordance with local clinical guidelines.	
4	Position the eye adequately. At an area of 1.0–2.0 mm posterior to the limbus, mark an injection site.	

For more information about EYLEA®, visit <https://ophthalmology.bayer.com>



Bayer AG, 51368, Leverkusen, Germany
Germany Copyright © 2026
PP-EYL_8mg-IE-0228
Date of revision: April 2026